

GQ GMC-500/GMC-500+ Geiger Counter User Guide



GQ Electronics LLC

Revision 2.0

Sep-2020

Document Revision History:

- Re 2.00, Aug-2020Added Dosimeter ModeRe.1.50, Sep-2018Content reviseRe.1.40, Sep-2018Content revise for hardware v2.00Re.1.30, Sep-2018Data saving related content revised.Re.1.20, Sep-2017Re.1.01, Apr-2017Re.1.00, Eth 2017Re.1.00 Eth 2017
- Re.1.00, Feb-2017

Table of Contents

User Guide	1
Table of Contents	
Overview	5
Specifications:	5
Packing List:	6
How it works?	
Caution	
Background Safe Levels	
Hardware setup	
Software set up	
Verify USB driver installation in Windows	
S1 key	
S2 key	
S3 key	
S3 keyError! Bookmark	
Power saving mode	
Popup Windows	
Graphic User Interface (GUI)	
Graphic Icons:	
Dual Display Modes	
Display Modes	
Graphic Mode:	
Text Mode:	
Large Font Mode:	14
User Option	
Alarm Set	16
Date and Time setting	17
Data Saving Setting	
Threshold Data Saving Setting	
Add Note or Add Location for data saving	
Note/Location Input	
Erase Saved History Data	
Display Option	
Swivel Display Option	
WiFi Setup and Check	
WiFi IP address	
WiFi Mac address	
WiFi Signal Level Checking	
Internet Data Server Setting	
Website server	
URL for Website server	
Website server User ID	
Website server Geiger Counter ID.	
WiFi Data Logging Period	
WiFi Data Logging Testing	
Calibrate the reading	
Tube Voltage (GMC-500 only)	
Tube Settings (GMC-500+ only)	
Select Tube Settings to change tube settings on GMC-500+	
Factory reset	
Battery Status	
Battery Type Error! Bookmark	
Power saving mode	25
Motion Detection	

Reset Total Count	
Gyroscope Data Display	
Communication Baud Rate	
Reverse Display	
Contrast Adjustment	
Timed Count	27
Set a schedule	27
Set Timed Count Duration	
Start a Timed Count	
About	
Model information	
Firmware version	
Unit serial number	
GQ GMC Data Viewer Software	
Online Geiger Counter World Map	
www.GMCmap.com	
Software	
Auto Submit Data Protocol	
Applications	
Stationary Application	
Other technical details you may want to know	
Data Port	
USB Port	
Data collection time	
Extend battery operating time	
Third party software developers	35

Overview

The.GQ GMC-500/GMC-500+ digital Geiger Muller Counter is designed to be a portable and convenient device. It can be used as industrial, commercial maintenance, research, evaluation, simulation and other analytical or scientific applications in areas such as industrial plants, public utilities, universities, laboratories, and electronic repair shops. The device comes with built in audible and visual signals for the level of radiation detected. It can be used for radiation detection and monitoring both indoor and outdoor, as well as in other similar environments. It features automatic data recording. It can continually monitor the radiation and log the data each second into internal memory. When connected to a PC, software can download the radiation history data to the computer and the user is able to analyze those data later. The GQ GMC-500 installed a high contrast black/white LCD module, one front LED indicator and one analog data port. The analog data port can be connected to any third party device application as data input.

The GMC-500 installed a Wi-Fi module, user is able to log the data via Wi-Fi wirelessly.

The GMC-500+ installed a second high dose sensor tube to ensure the detection range up to ten times higher.

The device is equipped with an USB port, utilized for communication and external power supply/charging of the internal rechargeable Li-Ion 3.6V/3.7V battery.

The internal rechargeable battery can be charged with the standard USB port, USB charger or with a computer USB port. Using the external power, continuous data monitoring is possible. Using either power adapter you will not have to worry about the batteries charge condition or any data loss.

The main board also has a real time clock on board for time related data logging purposes.

The GMC-500+ installed multiple sensors to ensure full scale/range measurement and higher accuracy. .

Specifications:

Range of dose rate indications, µSv/h	0.00 to ~4250
	(0.00 to ~42500 on GMC-500+)
Range of exposure dose rate indications, mRem	n/h 0.00 to ~425
	(0.00 to ~4250 on GMC-500+)
Range of registered beta radiation energy MeV	0.25 to 3.5
Range of gamma radiation energy, MeV	0.1 to 1.25
Range of registered X-ray radiation energy MeV	0.03 to 3.0
Gamma Sensitivity Co ⁶⁰ (cps/mR/hr)	23
Reproducibility of indication	10%
Alarm levels by CPM	0 to 655350 (continuously)
	0 to 982980 (GMC-500+)
Alarm levels by µSv/h	0.00 to 4250 (42500 on GMC-500+)
Alarm levels by mRem/h	0.00 to 425 (4250 on GMC-500+)
Date indication	YYYY-MM-DD (continuously)
Time indication	HH-MM-SS (continuously)
Elapsed time indication	99 years (maximum)
Timed Count	1 Second to 256 days (programmable)
Scheduled Timed Count	0 Second to 256 days (programmable)
Radiation detection	β, γ, ×
Detectable Radiation Range	0.1 ~ 3 MeV
Instrument Background Noise	< 3 pulses/s
Working Voltage	3.6-3.7V
Display	LCD dot matrix, back lighted
On board Memory	1M Bytes flash memory for data storage
Power: Consumption	25mW – 125mW (count rate dependent)
Power: Supply	3.7V Li-lon battery / USB power
	· ·

Dimensions

Packing List:

- 1. GMC-500/GMC-500+ main unit.
- 2. USB cable
- 3. Quick start guide
- 4. Download link for SoftGeigerCounter software and USB driver for Windows 32 and 64 bits (see Quick start guide)
- 5. Download link for a complete user guide in pdf version.

How it works?

The GQ-500/GMC-500+ Geiger Counter installed Geiger tubes to detect radiation.

When the radiation pass through the Geiger tube, it triggers electrical pulses for the CPU to register as count. The basic count rate unit is CPM (Count Per Minute). The CPM count rate indicates the radiation level and it can be converted to another traditional radiation units, such as μ Sv/h or mR/h.

After unit turned on for one minute, it will show the background radiation reading. The background radiation reading (in CPM) indicates the nature radiation detected at that minute. This reading may change from time to time and location to location. To get accurate reading, user may need to get an average value over a longer time period.

The GM-500 built-in intelligent algorithm always select one of the most adequate sensors to measure the target, so that to guarantee the accuracy of the measurement.

Caution

- 1. Avoid doing measurements when battery low.
- 2. Do not get the Geiger counter wet. Use sealed plastic bag to void wet.
- 2. Avoid doing measurements in direct sunlight.
- 3. Avoid directly contact the radioactive material. Use sealed plastic bag if needed.
- 4. Turn off the unit when not in use.
- 5. Keep it in a protective pouch after use.
- 6. When the unit not in use, store it in a dry place or box. This will avoid mechanical part be oxidized, such as button or battery contacting points.

Background Safe Levels

Suggested background readings levels:

1. **Safe level**. Less than 50CPM or 0.325µSv/h. Means no worry at all.

2. Attention level. 51 CPM – 99 CPM. OR 0.326μ Sv/h – 0.65μ Sv/h. Means you need to find out why.

3. **Warning level.** More than 100CPM or more than 0.65µSv/h. Means do not stay in this area for long period.

Hardware setup

There are four buttons on the front of the unit: S1, S2, S3 and S4 (from left to right)

- 1. Power up the unit. Pressing the S4 (power) key for 3 seconds will turn on the unit. Check the battery level. Charge the battery fully when first time use. It may take a few hours to get the battery fully charged. Check the battery icon on the display, a fully charged battery icon will be filled with solid color, without flashing.
- 2. Set date/time. Press the S4 key to enter the Main menu->Init Setup-> Date/Time submenu to set the date and time. This is very important for time stamping the recorded data. Do not skip this step. Most of the data are related to the date and time.
- 3. Set the backlight timeout from Main menu->Display Options->Backlight Timer sub menu. User may enable the power saving mode from Main menu->User Options->Power saving Mode sub menu. If the power savings mode is ON, then the LCD display will be turned off after 30 second if no key is being pressed during this period.
- 4. Now the unit is ready to use. You should see the background CPM rate in absence of a radioactive source.

Note: There is a transparent protective sheet covering the unit's surface. Users need to remove it to get better view of the LCD display.

Software

Before connecting the GMC-500/GMC-500+ Geiger Counter to a computer, download the application software and install the USB driver. Download these from: http://www.gqelectronicsllc.com.

- 1. The unit needs an USB driver in order to communicate with the application software. Running **GQGMCGeigerCounterUSBDriverV4.exe** will install the USB driver.
- 2. GMCDataViewer.exe is for viewing the data on a computer.
- 3. SoftGeigerCounterGMC500.exe is a soft copy of GMC-500 demo software.

For technical questions and support, please use the forum at the following link:


http://www.GQElectronicsLLC.com/forum

For the latest software, please visit our software download page:

http://www.ggelectronicsllc.com/comersus/store/download.asp

Verify USB driver installation in Windows

Once the GMC-500/GMC-500+ is connected to a computer, from the device manger, you should see which COM port is assigned to the unit. See the example below. Windows assigned COM3 to the GMC-500 unit in this example.

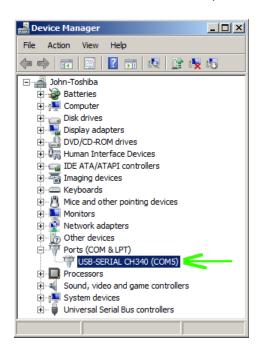


For the data viewer or the data logger software, selecting COM5 will establish the connection to the GMC-500 Geiger counter for the above example

0 5	10	15	20	25	30	35	40	45	50	55(Time)6	Peak
Play	×	a	Stop		E Re	ealtime Mo	nitoring			•	
COM7 opened si GMC-500Re 1.0											
GMC-500Re 1.0	- 1	on compo						_		•	
Downlo	ad		GMC-500		•	Сом7	·	-	_	Exit	
GQ Geiger Muller Counter Data Viewer About											
				V.	2.34						

GQ GMC Geiger Counter Multi-Function Keys

The multi-function keys S1, S2, S3 and S4 explained:





Vertical Display Mode

Horizontal Display Mode

These key's function will be reassigned dynamically based on the context of the current (sub-) menu being displayed.

S1 key

- 1. There are three display modes: Text, Large Font, Dosimeter, Graphic, and Food Mode. Pressing the S1 key toggles between these modes.
- 2. In the menu screen, pressing the S1 key will exit the current menu and will return back one menu level.
- 3 In the data input mode, pressing the S1 key will delete the last character entered.

S2 key

- 1. In text mode, pressing the S2 key will change the text information format.
- 2. In graphic mode, the S2 key will increase the graphic ZOOM factor.
- 3. In menu mode, the S2 key acts as the UP key to move the highlight menu item upwards.
- 4. In the menu mode, while a popup message box is opened, the S2 key changes the value by cycling through the predefined values.

S3 key

- 1. In text mode, pressing the S3 key will change the displayed date/time selection.
- 2. In graphic mode, the S3 key will decrease the graphic ZOOM factor.
- 3. In menu mode, the S3 key acts as the DOWN key to move the highlight menu item downwards.
- 4. In the menu mode, while a popup message box is opened, the S3 key changes the value by cycling through the predefined values.

S4 key

- 1. In power off state, only the S4 key acts as the power switch. Holding it for 3 seconds will power up he unit.
- 2. In power on state, holding S4 key for 3 seconds will switch the unit off.
- 3. In menu mode, S4 is the "Confirm", "Select", "Enter" key

Power saving mode

The unit's factory default power saving mode is ON. In this mode, the unit will turn off the display after 30 seconds idle time. It turns on the LCD display when any key is pressed.

Popup Windows

The Popup Windows will show the current status/value of selected features. The current status/value can be changed only when it is displayed in the Popup Window and the currently displayed status/value will be stored when the Popup Window has timed out after 3 seconds if no key has been pressed.

08-	-09-2013 J	العشر
CPM	Text Mode	i∕h
Tot		

Graphic User Interface (GUI)

Graphic Icons:

auto	Graphic ZOOM factors: 0.5, 1.0, 2.0, AUTO
	Battery Status.
Ψ	Data saving enabled / (History data)
Ň.	Alarm enabled
40	Sound enabled
œ	Timed Count. It flashes if timed count in progress.
Ê.	Wi-Fi Connection
X3.0	Current graphic ZOOM factor
CPM:	Current CPM reading
ΨCΡΜ	History CPM reading
Total	Count: Total count since power on OR reset/clear.



Average CPM of a specific time frame.

Maximum CPM:

Maximum CPM since power on.



Current radiation level is normal.



Current radiation level is medium.



Current radiation level is high.

Dual Display Modes


GMC-500 supports two display formats to fit user's display preferences: Vertical Display and Horizontal Display.

With the Horizontal Display, the user can select one information screen from: **Text, Graphic, Large Font** or **Menu**. The Vertical Display Mode displays **Large Font mode**.



Vertical Display

Horizontal Display

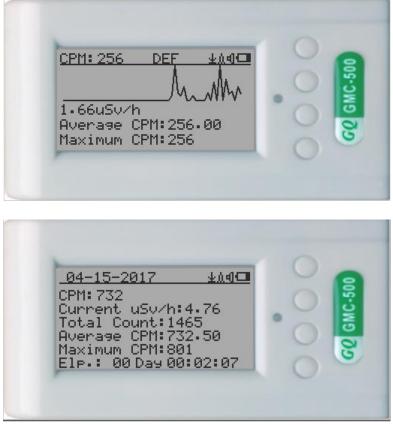


Horizontal Displays

Display Modes

There are six ways to display the information, Large Font Mode, Dosimeter Mode, Text Mode, Graphic Mode, Food/Sample Mode, and Timed Count.

Graphic Mode:

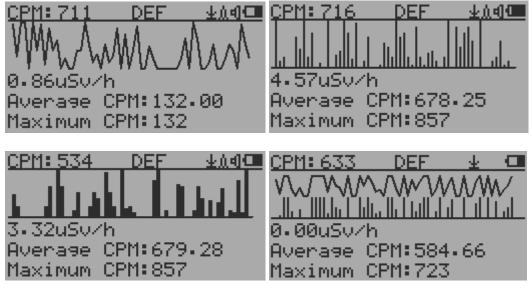

CPM: 606

Current radiation level reading in CPM format (Counts Per Minute)



CPS (Count Per Second) in last 60 seconds.

Text Mode:

04-06-2017	<u>⊉≬d⊡</u>
CPM: 232	
Current uSv	
Total Count	
Averase CPM	
Maximum CPM	
Elp.: 00 Day	100:00:25

04-06-2	017		<u>+14</u>
CPM: 601			
Current			91
<u>Total</u> Co			
Averase.			99
Maximum			
Elp.: 00	Day.	00:0	1:26

08-09-2013	15:29:36
00 07 2010 .	

CPM: 554	
Current	uSv/h:4.95
Current	mR/h:0.414

<u>13:49:53</u><u>40</u>⊂ CPM:618 Total uSv/h:3.65 Total Count:1123 Average CPM:561.50 Maximum CPM:654 Elp.: 00 Day 00:01:55

13:50:18	±∆d⊡
CPM: 625	
Total mR/h:0.453	
Total Count:1395	
Average CPM:697.	50
Maximum CPM:654	
Elp.: 00 Day 00:0	2:20

Current date and time (Press S3 for toggling between date and time) Current radiation level reading in CPM Current radiation level in µSv/h or

mR/h format

Total Count:10052 Total mR:0.432

Total uSv:4.26

Maximum CPM:30

Total count.

Total cumulated radiation dose in mR since power on.

Total cumulated radiation dose in uSv since power on.

Elapsed time since power on (Press S2 for toggling displayed info) Maximum CPM since power on Average CPM since power on.

Navigation keys for both modes: S1: Text/Graphic Display Mode Selection

S2: μ Sv/h, mR/h, Total Count, Elapsed Time selection


S3: Date or Time on title selection

Elp.:00 Day 00:16:34

Average CPM:28.25

S4: Menu

Large Font Mode:





08-09-2013,15:29:36

Current date and time (Change it in Text Mode) S2 key toggles between CPM, μ Sv/h and mR/h mode

Navigation keys:

S1: Text/Graphic/Large Font Display Mode Selection

689

0.448 mR/

CPM

- S2: μ Sv/h, mR/h, CPM selection \rightarrow
- S3: μ Sv/h, mR/h, CPM selection \leftarrow
- S4: Menu

NOTE: Large Font Mode is available in firmware Ver. 2.20 or later only

Dosimeter Mode:

CPM: 15	业血和
Dose(µSv)	0.0037
Rate(µSv/h) 👘	0.0975
θye (µSy∕h) —	0.1473
Alarm(µSv)	0.9999
	00:01:30
· <u>- · ·</u> - · · · · · · · ·	0 <u>6:45:4</u> 2
- SECHANGE UNIT	BBRESET-

Navigation keys:

- S1: Display Selection Mode
- S2: μ Sv/h, mR/h, CPM selection \leftarrow
- S3: Reset dose S4: Menu

Food/Sample Testing Mode

<u>Time 0±0 0</u> Step #1: Select duration: 🖴	T bet cor
<u>05</u> minutes ▲: Next ▼: Change time	The Do pro
<u>Sample 1</u> Step #2: Put Device Close To Sample 1 (Back9round) ▲: Start ▼: Use previous data	
<u>Sample 2</u> <u>0±≬</u> Step #4: Put Device Close To Sample 2 (Sample)	9

Use previous data

0.00 CPM

0.00 µSv/h

#1

0.00

0.00

ፀቋል 🚥

#2

0.00 0.00 This mode can be used for comparing radiations between two samples. It can be also be used for comparing food radiation to the background.

The first step is choosing the time duration. Pressing the Down Button will update the time, and S3 button to proceed.

Sample 1	ወ±ሲ	1
Step #3: Colle	cting	
data, please	wait.	
00:04:57	12	
)	

Sample 2	ፀቋል ወ
Step #5: Colle	cting
data, please	wait.
00:04:36	8%

Step 2-5 is for collecting radiation data between samples.

Results screen will popup after step 5 is finshed.

The data collecting process can also be canceled by pressign the S2/Down Button.

▲: Start

<u>Results</u>

05 mm.

JSV∕h

Jar.

CPM

Start

Menu Display

Main Menu

Main Menu	业创团	Main Menu	业魚创⊂■
→User Option		Timed Count	× .
Display Option		- WiFi	
Save Data .		Şerve <u>r</u>	
Timed Count		Init Setup	
WiFi		Others About	
Server		→Exit	
Init Setup	\sim	7EXIU	

Navigation keys:

S1: Back S2: Up S3: Down S4: Select/Enter

User Option

<u> User Option </u>	
→Speaker	
Alarm	
LÉD Indicator	
Power Saving	
Motion Detect	
Reset Total Count	
Exit	

Navigation keys:

S1: Back S2: Up S3: Down S4: Select/Enter


Alarm Set

Alarm	💻 ውስቋ
⇒On∕Off	
CPM(*)	
usv	

CPM(*)

Currently the CPM alarm mode is selected The audio alarm will be triggered once the radiation level reaches the preset alarm threshold.


Date and Time setting



Navigation keys:

- S1: Back/Exit
- S2: Increase value by 1 (or hold the key down)
- S3: Decrease value by 1 1 (or hold the key down)
- S4: Select setting mode between Year, Month, Date, Hour, Minute and Second. Each key press will change the mode to be set.

NOTE: Setting of Date and Time is important, all history data use Date and Time as a time stamp reference.

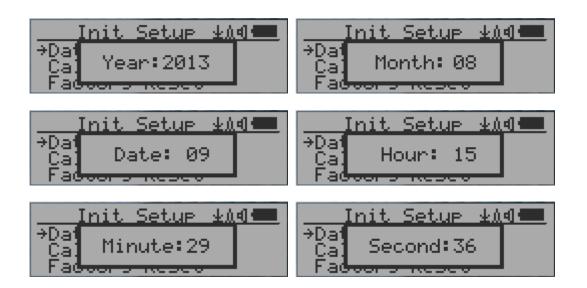


NOTE: you need to set the seconds to let unit complete the date & time setup.

Data Saving Setting
Save Data ±∆d →Save Mode Note/Location History Data Threshold Erase Saved Data Exit
Threshold ∳ú¶⊡







Selecting this item will turn on/off the real time data saving from followings:

OFF -> Every Second ->Every Minute -> Every Hour->Every Second Threshold->Every Minute Threshold

NOTE: The history data memory will be used as a ring buffer. Once the end of the memory is reached, the oldest data will be over written. Carefully select the data saving interval to save memory space.

With Threshold saving mode, data only will be logged if it exceed the threshold value.

The data will not be logged while viewing history data in the History Data menu.

Threshold Data Saving Setting



Select threshold type you want to use: CPM, uSv OR mR



Add Note or Add Location for data saving

Save Data	业加创📟
Save Mode	
→ <u>N</u> ote/Location –	
Threshold	\sim

The user may add a note with up to 16 characters into the history data to identify the measurement or location.

This note/location information will be saved together with the radiation data.

Note/Location Input

Note/Location	<u>+04</u>
HOME_	
_	


The cursor indicates the position of current character input.

Navigation keys:


S1: Backspace and erase S2: Move cursor right \leftarrow S3: Move cursor left \rightarrow

S4: Exit & Store

Erase Saved History Data

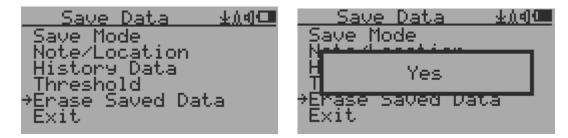

Use S2 and S3 to select Yes or No on the screen to confirm the request. After about 3 seconds with Yes confirmation, the unit will start to erase entire saved history data. It may take a few seconds to complete the task.

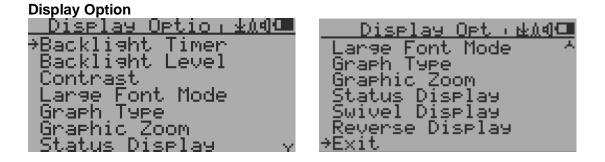

Swivel Display Option



Pressing the S4 key will cycle between: Normal -> Swivel -> Auto Swivel modes

In the Auto Swivel mode, the display will be rotated by 180° if the unit is held upside down.

Wi-Fi Setup and Check

The Wi-Fi tested with 802.11 n, 802.11 g/n, 802.11 b/g/n under WPA2-PSK (AES), WEP, WPAWPA2-PSK (TKIP/AES) and Open security modes.

Main Menu	业创制	WiFi y	e de la
User Option		→WiFi On∕Off SSID	
Display Option Save Data		Password	
Timed Count		WiFi Signal	
→WiFi Server		IP Address Mac Address	
Init Setup	Y	Reset WiFi Modul	e v

Select Wi-Fi On/Off item will turn the Wi-Fi connection On/Off

Make sure the Wi-Fi SSID and Password have been set.

Note: All Wi-Fi settings available from GQ GMC Data Viewer Windows software for easier and faster setup.

Wi-Fi IP address



Wi-Fi Mac address

<u> </u>		WiFi 🔬 🖛
- <u>WiFi</u> On∕Off		WiFi On/Off
SSID		SCIP.
Password WiFi Signal		[]1f.13.5f.2e.9d.11
IP Address		Îr Rooress
→Mac Address		→Mac Address
Reset WiFi Module	\sim	Reset WiFi Module 🗸

Wi-Fi Signal Level Checking

WiFi	生血的	<u> </u>	<u>+04</u>
Password →WiFi Si⊜nal	×.	Pas -55	5dB
IP Address	×.	IP HOG COD	

Internet Data Server Setting

This menu setup is mainly for a data logging server. The unit data can be logged to a server automatically via Wi-Fi internet HTTP connection.

Here is the default website server setup for: www.gmcmapcom

Website server

User is able to change the server name to point to another http server.



URL for Website server

The default web server data receiving URL is log2.asp.

User is able to change the URL to user specific URL. However, the URL data parameters in a fixed format.

Example:

http://www.GMCmap.com/log2.asp?AID=0230111&GID=0034021&CPM=15&ACPM=13.2&uSV =0.075

Server	<u></u>	URL	<u>+04</u>
Website →URL		1092.asp_	
Üser ID	\sim		

Website server User ID

Each data submission has a user ID. The user ID is the user account ID from the data server. It will send to server with the data to log.

This is an example user ID from www.gmcmap.com

Server	<u></u> 0.01	User ID	<u>ውስታ የ</u>
URL	A	002342_	
→User ID Counter ID	~	_	

Website server Geiger Counter ID

Each data submission has a Geiger Counter ID. The Geiger Counter ID is a unique ID in data server database. It will send to server with the data to log. This is an example Geiger Counter ID from www.gmcmap.com

Server	<u>+104</u>	Counter ID	<u></u>
User ID →Counter ID	<u>^</u>	3245215387_	
Period	\sim		

Wi-Fi Data Logging Period

The default data logging period is 2 minutes. This will let unit to log the data to website server every two minute.


User is able to change the period from 1 to any minutes.

Server 🚽	1d) 🛄	Period	<u>+101</u>
Counter ID →Period	<u> </u>	2_	
Test Connection	×.		

Wi-Fi Data Logging Testing

User can test the server settings anytime to confirm the server settings are working.

The result will be either Successful or Link Server Failed.

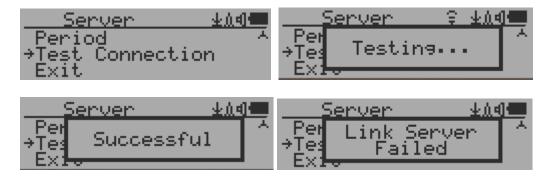

Note: All Server settings available from GQ GMC Data Viewer Windows software for easier and faster setup.

Calibrate the reading

The unit has been calibrated in factory. In most of case, the re-calibration is not necessary. However, you can calibrate the unit with a standard radiation sources.

The factory default calibration value is for general in-door and out-door measurements.

Calibration



Select Calibrate form the Main Menu. There are three points provided for calibration.

Calibrate	<u> </u>
⇒Calibrate 1	
Calibrate <u>2</u>	
Calibrate 3	

Each calibration point needs two values to be entered, the CPM value and the μ Sv/h value. The user can enter up to three calibration points from large to high count rates.

Procedure:

- 1. Place the testing radiation source ~30mm away to the center of unit Geiger Tube side. In Text or Graphic mode, wait for at least 3 minutes.
- 2. Note the CPM value.
- 3. Select Calibrate menu item on the device, then input both the CPM value you noted and the known μ Sv/h value of the calibration source.
- 4. Wait for the popup window to close to save the data for this calibration point.
- 5. Continue with step 1 with other calibrated radiation sources.






Navigation keys:

- S1: Back/Exit
- S2: Increase the value by 10 CPM or 0.1µSv/h respectively
- S3: Decrease the value by 1 CPM or 0.01µSv/h respectively
- S4: Toggle input data type between CPM and μ Sv/h

Tube Voltage (GMC-500/600/600+)

The menu allows advanced user to configure a specific sensor tube voltage.

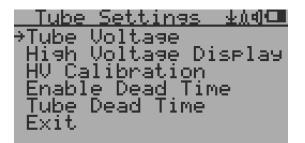


Tube Voltage: about 3 to 600V, Steps: 1 to 100, the voltage change is not in linear. High Voltage Display: Display high voltage reading in Text Mode HV Calibration: For adjusting the high voltage reading Enable Dead Time: For including tube dead time in the CPM calculation Tube Dead Time: Dead Time Value

Tube Settings (GMC-500+ only)

The menu allows advanced user to configure a specific sensor. User also allows to change the two tubes voltage independently. The functions are the same as mentioned above but with also an option for the 2nd tube.


Select Tube Settings to change tube settings on GMC-500+ under Init Setup.

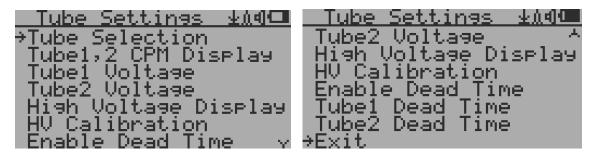

Tube Selection allow user to select the active tube: #1 high sensitivity tube, #2 high dose tube or both

Tube1, 2 CPM Display enables individual tube readings on large font mode screen. Tube1 Voltage: about 3 to 600V, Steps: 1 to 100, the voltage change is not in linear. Tube2 Voltage: about 3 to 600V, Steps: 1 to 100, the voltage change is not in linear.

Factory reset

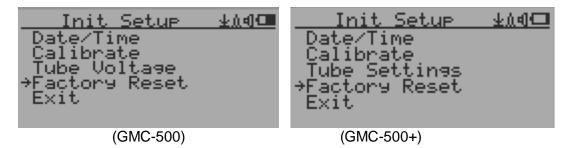

Select Factory Reset to reset the unit to the factory default settings.

Note: The reset will erase all user settings and recorded history data.



Procedure:

Select Factory Reset menu item and change the popup Windows message to Yes. Wait for popup message window's timeout to confirm the reset request. Any other key press will cancel the reset request. It may take up to 30 seconds to complete the reset.

Battery

Can be found under 'Others' menu. It displays the current battery voltage.

Power saving mode

User Option 🗚 🕮
Alarm
⇒Power Savina
Motion Detect

Pressing the S4 key will toggle the Power Saving mode ON and OFF.

In power saving mode, the units LCD display will be turned off after 30 seconds if no key is pressed to save battery power. The audio signal will not be turned off if it has been set to ON. The LCD back light will be off during the power saving mode.

Pressing any key will active the LCD backlight again.

The unit movement does not weak up the unit if the motion detection is OFF.

Motion Detection

User Option 🗚 🕮
Power Saving
⇒Motion_Detect
Reset Total Count



GMC-500 has motion detection feature. It can detect unit movement, upside down, single tap and double tap. Turn off the motion detection disables all motion related features.

Reset Total Count



This may be used before a fixed time count measurement start.

The Reset Total Count menu item let user to clear the total count on main text mode screen.

t.

Gyroscope Data Display



The internal digital accelerometer is able to provide real-time gyroscope data. It displays current unit X, Y, Z axis data and detected motion event. Such as single tap OR double tap.

Communication Baud Rate



This Geiger counter serial communication baud rate is selectable from following value: 1200,2400,4800,9600,14400,19200,28800, 38400, 57600, and 115200. Press S4 key changes baud rate.

The new baud will take immediate effect. The new value also be saved and used on next power up.

Reverse Display



Contrast Adjustment



Use S2 and S3 to adjust the contrast level. The contrast level will be saved and it will be used when the unit is ON.


Timed Count

The Timed Count can be started with a schedule OR without a schedule.


When it started with a schedule, the Timed Count will be started after a scheduled time period passed. This is useful if a testing target is not ready immediately.

When it started without a schedule, the Timed Count will be started immediately once the timed count period is set.

The Timed Count can be set from the menu:

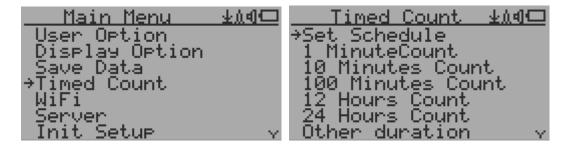

Set a schedule



This example shows the schedule is set to 2 minute.

Navigation keys: S1: Back/Exit

- S2: Increase the cursor position value
- S3: Decrease the position value.
- S4: Move the cursor to input data type between Day, Hour, Minute and Second.

Set Timed Count Duration

There are 5 preset durations from menu: 1 minutes, 10 minutes, 100 minutes, 12 Hours and 24 Hours.

If the duration is not listed, then you can set a new duration (1 second to 256 days) from menu 'Other duration':



This example shows a 2 days duration is set for Timed Count.

Navigation keys:

- S1: Back/Exit
- S2: Increase the cursor position value
- S3: Decrease the position value.
- S4: Move the cursor to input data type between Day, Hour, Minute and Second.

Start a Timed Count

If no Schedule set, then the Timed Count starts immediately after the duration set.

If the Schedule is set, then the Timed Count will be started after a scheduled time period passed. This is useful if a testing target is not ready immediately.

Once the Timed Count schedule is active, the Timer icon will be showed on the top icon area.



When the Timed Count started, the screen will pop up a message: Timed Count Started.

<u> Timed Count ±∆4⊂</u>	Time
Set Schedule	→Cancel Exit
i Timed Count i Started!	EXIC
1 2 Hours Count 24 Hours Count	
Other duration 🗸 🗸	

Count

Յերվա

The Timed Count can be cancelled anytime.

Now you can exit the menu and see the Timed Count progress screen and information:



About


This menu item is used to gather information about the instruments model number, firmware revision and serial number.

Main Menu	<u>0±11</u>	About	<u> </u>
<u>Tim</u> ed Count	~	→Model	
<u>M</u> iFi		Revision	
Server		Serial #	
Init Setup		Manufacture	
Others →About		Exit	
Exit			


Model information



Firmware version




Unit serial number



GQ GMC Data Viewer Software

The GQ MGC Data Viewer software is a utility software comes with the GMC-500 package.

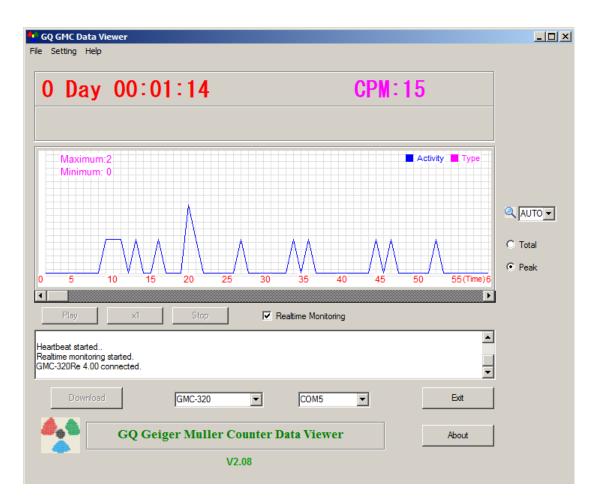

Main features:

- Download the history data from GMC-500
- Real time monitoring with graphic when it connected with GMC-500
- Save the history data in .bin OR .csv MS Excel format.
- Synchronize the data and time to GMC-500 with computer's data and time
- User defined automatic date and time synchronization period.
- GQ Terminal feature provide a detailed communication protocol exercise interface.

WiFi Setup Utility

With Data Viewer software Settings menu, users are able to quick and easily setup the device WiFi connection and data logging.

Settings			×
	Date Time Sy	nchronization W	ith PC
Auto Syr	nc Period: 1	Hours	Sync Date Time Now
	(O for disable a	auto sync)	Get Time From Unit
	Auto detect device	when start up so	oftware
	Geiger Cour	nter WiFi Data S	etup
SSID:	CenturyLink6993	Password:	11223CBBAA
Webite:	www.gmcmap.com	URL:	log2.asp
User ID:	33425	Peroid:	5
Geiger Co	ounter ID: 456542422		
Read	From Geiger Counter	Wr	ite to Geiger Counter
	Cancel	ОК	

GQ Terminal

5Q Terminal			[
Comport information: COM7, 115200,	n,8,1		Reconnect
Received in Hex Value:			
47 4D 43 2D 33 32 30 52 65 20 34	2E 30 39		Clear
Received in ASCII text:			
GMC-320Re 4.09			Clear
Last command in hexadecimal bee 3C 47 45 54 56 45 52 3E 3E			
	neters in hexade	cimal (E.g. C	
< GETVER			>>
Send com	hand with param	eters	
К	ey commands —		
Key1 (S1) Key2 (S2) Ke	y3 (S3)	Key4 (S4)
	Calibration ——		
Example #1	#2#3	Hea	id From Unit
CPM: 60 60 2	40 1000		5535 CPM
uSv: 0.05 0.30	20 5.00	Wri	ite To Unit
			Exit

The GQ Terminal provides an immediate access interface to the GMC-500 communication protocol.

Followings are click to send commands in software, for not listed commands user can type into the command box of software:

GETVER, GETSERIAL, GETCPM, KEY0, KEY1, KEY2, KEY3, SPEAKER0, SPEAKER1, ALARM0, ALARM1, GETVOLT, GETGYRO, GETCFG, GETCPS, GETTEMP, HEARTBEAT0, HEARTBEAT1, GETDATETIME, CFGUPDATE, POWEROFF, POWERON, SETDATETIME, FACTORYRESET

For detailed communication protocol commands, please see:

http://www.gqelectronicsllc.com/downloads/download.asp?DownloadID=62

An optional software is the GQ GMC Data Logger PRO. It is a generic software for different brand and model Geiger Counters. It has much more advanced features for advanced users.

See download page for the demo version.

Online Geiger Counter World Map



www.GMCmap.com

The Geiger Counter World Map is free and open protocol map. Anyone can use it for free. It provides a free space to all Geiger Counter users.

As a registered user, each user can have multiple Geiger Counters at different locations. All registered Geiger Counters have free history data storage space. User is able to retrieve their history data anytime, anywhere. User is able to publish their history data to others by set the data properties.

Software

The GMCmap accepts any software automatically submitted data.

The following tested software are free for automatic submit data feature.

GQ Geiger Counter Data Logger PRO (works on all Geiger Counter)
GQ Geiger Counter Data Viewer (works on GMC-300, GMC-320, GMC-500 series Geiger

Counters)

Both software can be found and downloaded from GQ Electronics LLC download page

The GMC-500 series is able to submit the data via internal Wi-Fi connection without other software.

Auto Submit Data Protocol

In order to use automatically submit data, user has to be registered from GMCmap.com, so that to get a valid user account ID and Geiger Counter ID. Each user can have multiple Geiger Counters at the different locations.

Auto submit data URL format:

http://www.GMCmap.com/log.asp?id=UserAccountID+GeigerCounterID+CPM+ACPM+uSV

At least one reading data has to be submitted.

Here: 1. UserAccountID: user account ID. This ID is assigned once a user registration is completed. 2. GeigerCounterID: a global unique ID for each registered Geiger Counter. 3. CPM: Count Per Minute reading from this Geiger Counter. 4. ACPM: Average Count Per Minute reading from this Geiger Counter(optional). 5. uSv: μ Sv/h reading from this Geiger Counter(optional).

Followings are valid data submission examples:

- 1. http://www.GMCmap.com/log.asp?id=0230111+0034021+15+13.2+0.075
- 2. http://www.GMCmap.com/log.asp?id=0230111+0034021+15+13.2+0
- 3. http://www.GMCmap.com/log.asp?id=0230111+0034021+15+0+0
- 4. http://www.GMCmap.com/log.asp?id=0230111+0034021+0+13.2+0
- 5. http://www.GMCmap.com/log.asp?id=0230111+0034021+0+0+0.075

The result will be returned immediately.

The following are the returned result examples:

1. OK.

- 2. Error! User is not found.
- 3. Error! Geiger Counter is not found.
- 4. Warning! The Geiger Counter location changed, please confirm the location.

If a location change warning received, the user need to confirm the location from that Geiger Counter profile. OR Create another Geiger Counter from your account. In this case, you can have two locations share one Geiger Counter.

Applications

Stationary Application

The unit has two holes on its back for hanging the unit on the wall for stationary monitoring of radiation and long term surveillance applications. With the wall adapter, it is able to monitor the data continuously, 24/7.



Mobile Application

To use the unit n the car while driving, use a car USB power adapter to charge/power the unit. Position the unit where it can easily detect radiation, i.e. on the dashboard or similar locations in the car. You may need to fix the unit to an appropriate location for safety reasons.

Other technical details you may want to know

Data Port

This model has a 3.5mm analog data output port. It uses standard 3.5mm audio stereo plug, This port is not for the earphone. The audio signal is for third party device and software. The signal can be connected to other devices or computer microphone port directly.

USB Port

The USB port is the standard mini-USB port. It is used for data communication, external power and the battery charger connection.

Data collection time

The GMC-500 radiation data is collected continuously, and every second the measured data is being transmitted to the CPU for processing.

Extend battery operating time

Turn on the Power Saving mode to extend the battery operating time. Turn off the speaker if it is not necessary. If a fully charged battery run-out in less than 5 operating hours, then the battery needs to be replaced. Use a standard 18650 (18 x 65.0 mm) rechargeable Li-ion battery.

The GMC-500 will operate normally when a non-rechargeable battery is installed. Select the battery type to none rechargeable battery from the unit menu.

Third party software developers

The GMC-500 is an open application protocol product. Users are able to develop their own software based on the published GQ-RFC1201 protocol. We encourage you to share your generic software with other users. Please contact support@gqelectronicsllc.com if you have any questions.

You can find the GQ-RFC1201 protocol at the software download page.

http://www.gqelectronicsllc.com/comersus/store/download.asp